




# Physicians Experience Breaks in the Cold Chain of Heat Sensitive Products

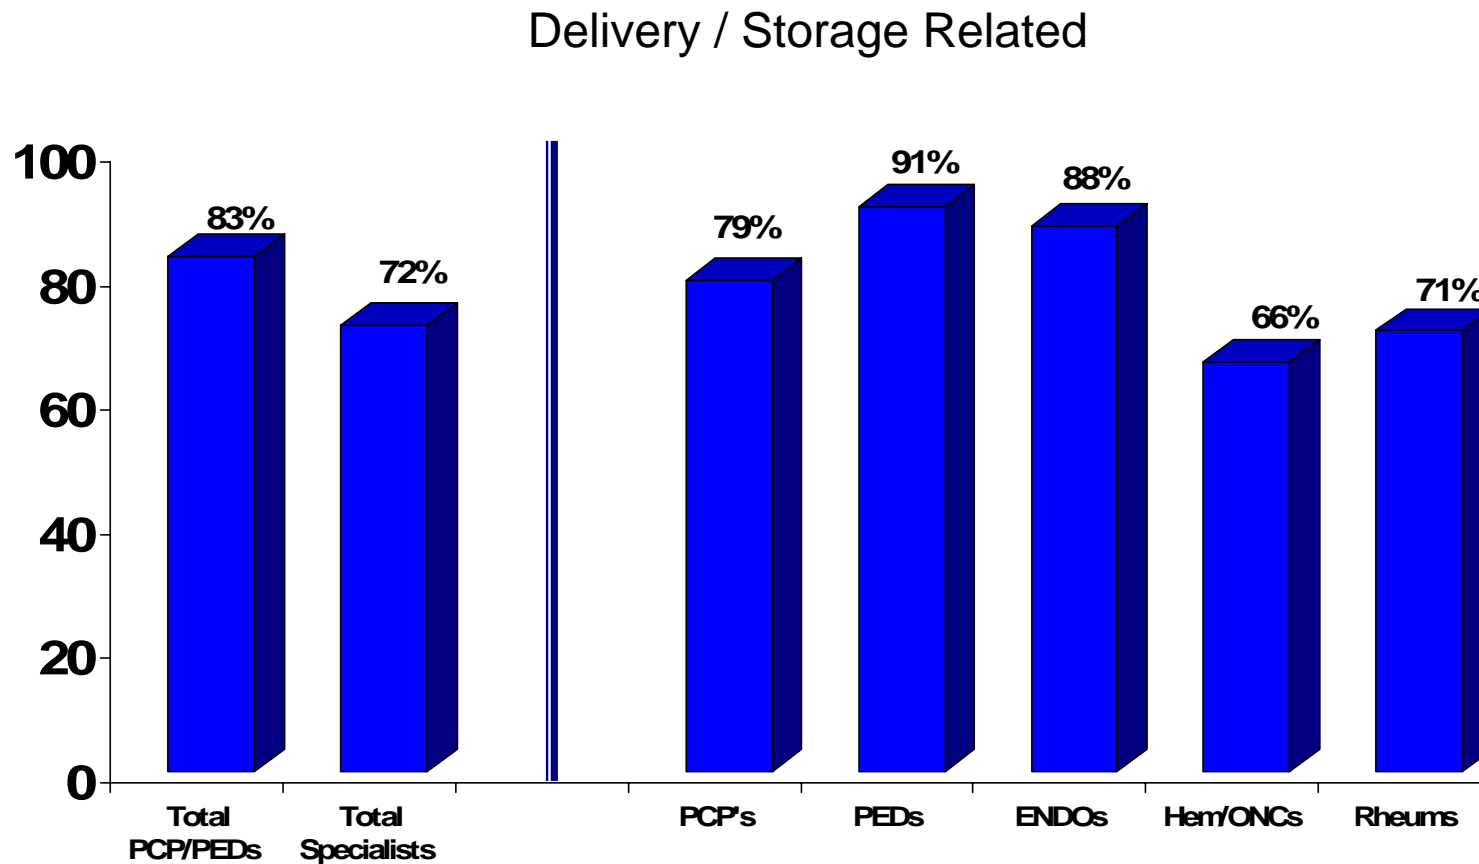

# Physicians Have Concerns About Products Losing Efficacy from Heat Damage

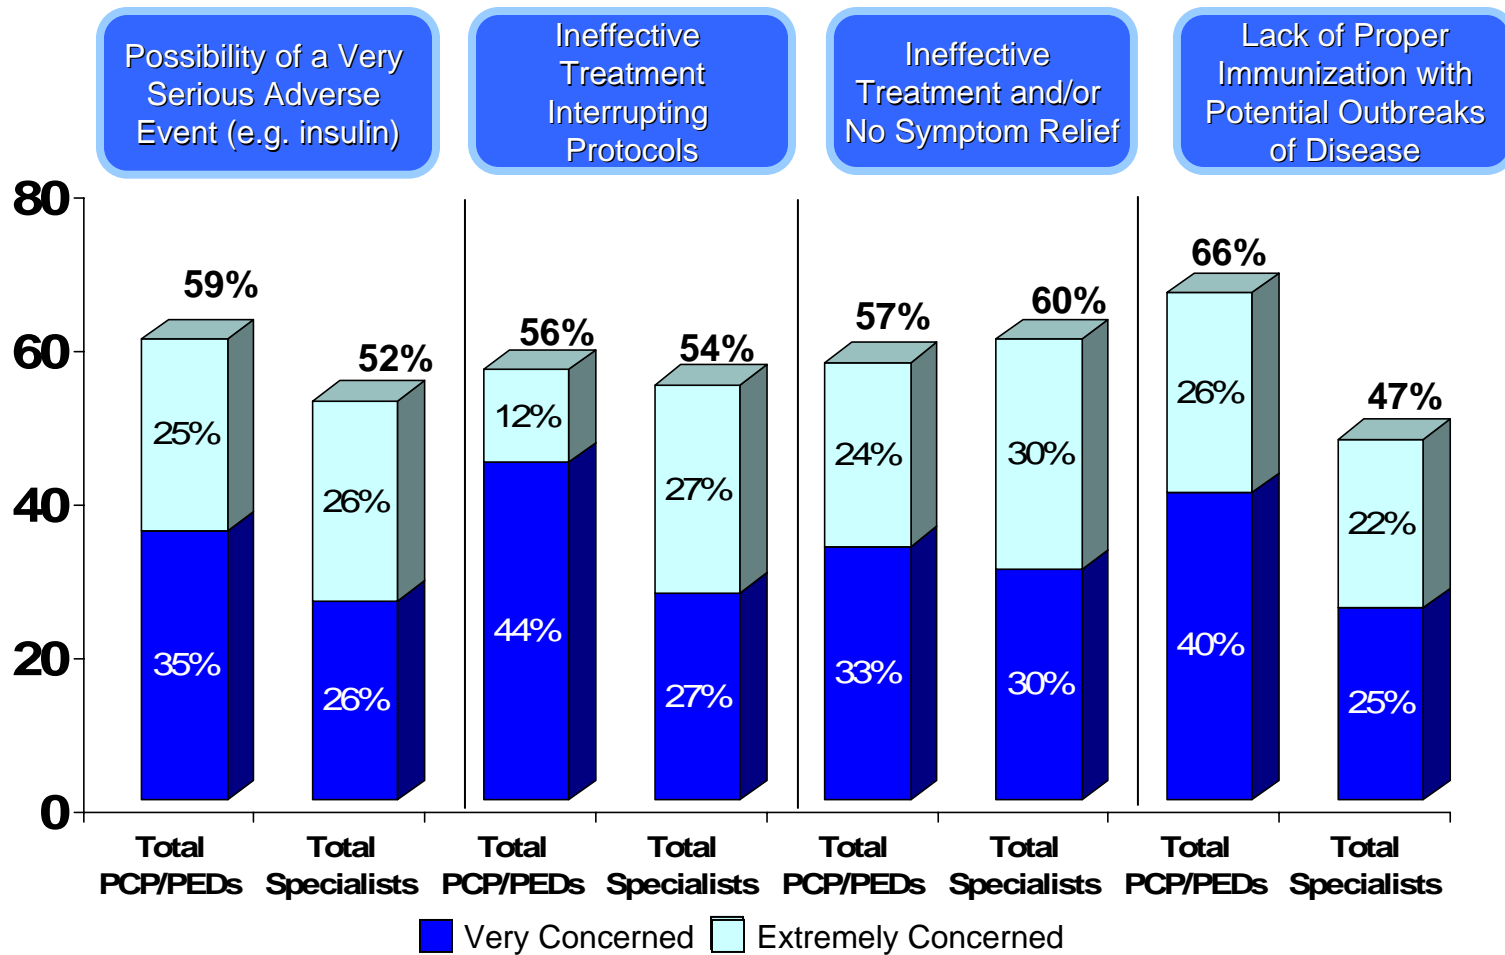


# Physicians Are Interested in a Device that Monitors Individual Units of Product from Manufacturer to Patient Administration\*

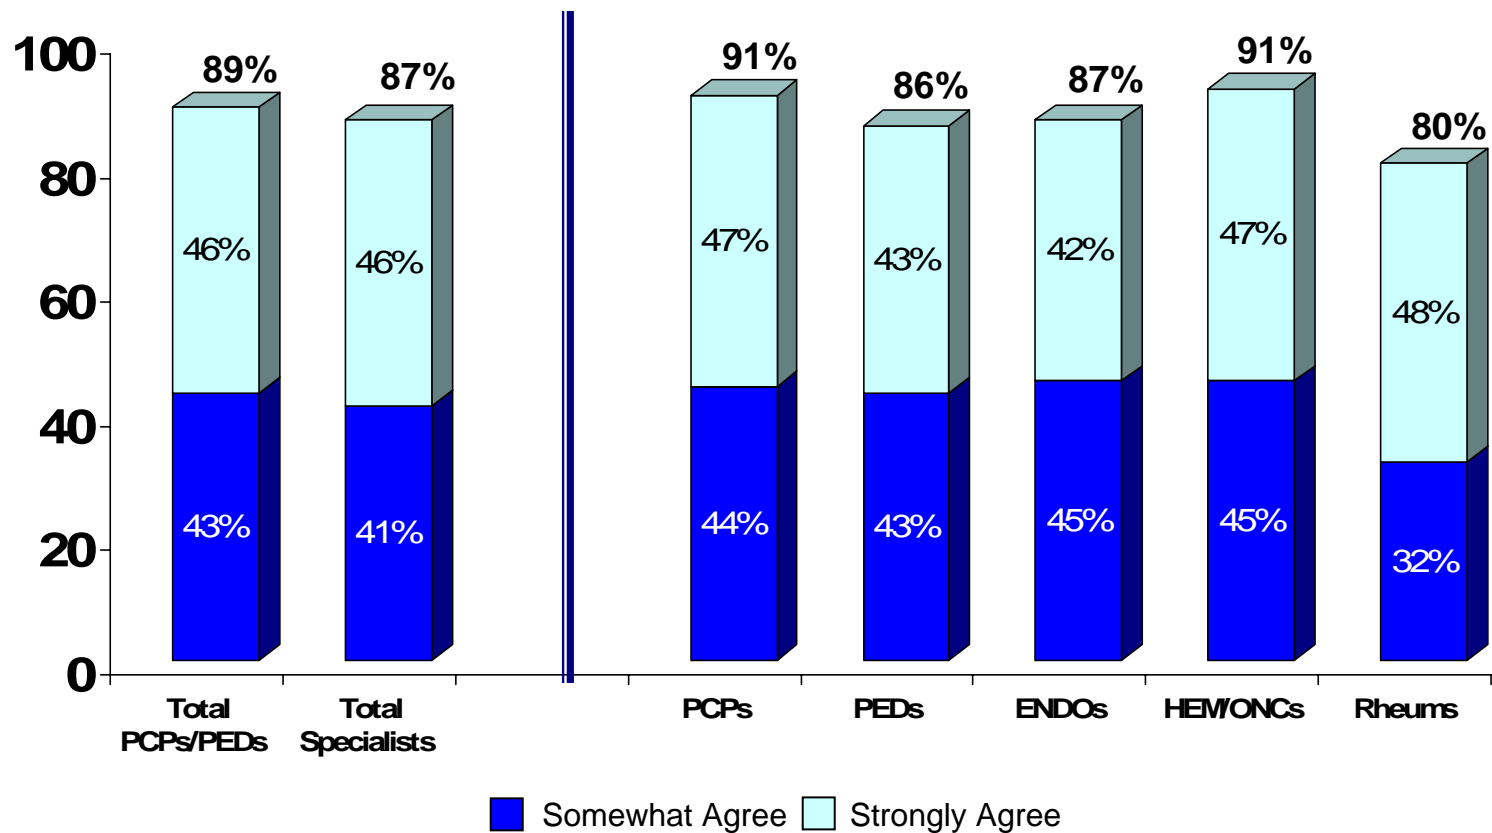

\* Physician Responses Prior to Exposure to HEATmarker

Source: Harris Interactive Physicians Quantitative Research Study, 2009; n=251 (Q.625)

# Physicians' Overall Impressions of HEATmarker® After Product Exposure Is Positive/Very Positive

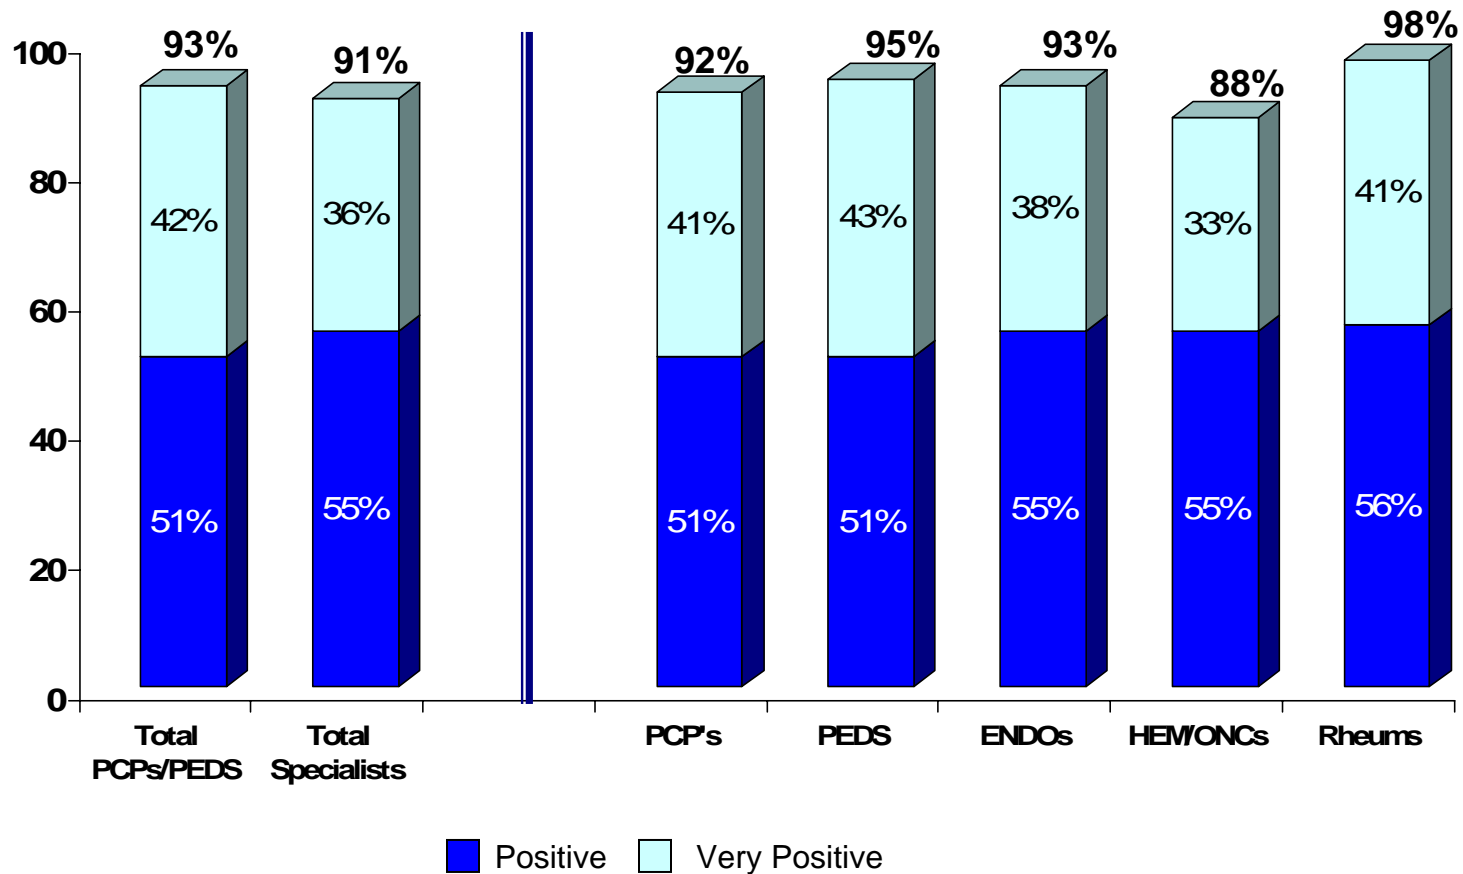

Source: Harris Interactive Physicians Quantitative Research Study, 2009; n=251 (Q.710)